

Impact of crown-to-implant ratio of marginal bone loss around implant-supported single crowns. A 5 years retrospective study

> **B. STOICHKOV¹, D. KIROV²**

¹DDS, PhD - Assistant professor, Department of Oral and Maxillofacial surgery, Faculty of Dental Medicine, Medical University, Sofia, Bulgaria

²DDS, PhD - Assistant professor, Department of Prosthetic Dentistry, Faculty of Dental Medicine, Medical University, Sofia, Bulgaria

TO CITE THIS ARTICLE

Stoichkov B, Kirov D. Impact of crown-to-implant ratio of marginal bone loss around implant-supported single crowns: 5 years retrospective study. *J Osseointegr* 2020;12(4):706-710.

DOI 10.23805 /JO.2020.12.01.05

ABSTRACT

Aim The success of implant-supported restorations depends on the stability of osseointegration and the amount of bone-to-implant contact. The aim of the present study is to assess the influence of the crown-to-implant ratio on marginal bone loss in prosthetic restorations with single implant-supported crowns.

Materials and methods Retrospectively, 65 patients with one missing tooth in the mandibular molar area were collected. All prosthetic restorations were made with single crowns, and all implants used were "bone level" type having a diameter in the range of 3.9 to 4.0 mm and a length of 10.0 to 13.0 mm. Cone beam computed tomography (CBCT) were performed in central occlusion. The height of restorative space was measured over the cross-sections from the level of the alveolar ridge to the corresponding antagonist crowns. Available bone height, width and length were also evaluated prior to implantation. Marginal bone loss was measured on pre-calibrated periapical radiographs, using ImageJ 1.52 (National Institutes of Health, Bethesda, Maryland, USA), in third and fifth year after the functional load.

Results Positive linear correlation, statistically significant, has been determined between the crown-to-implant ratio and the amount of crestal resorption. The highest peri-implant bone loss was recorded in cases with crown-to-implant ratio of 1.5/1 and higher.

Conclusion The results of this study indicate that prosthetic restorations with higher crown-to-implant ratio tend to cause higher marginal bone loss than those with lower one, in the mandibular molar area.

KEYWORDS: Crown-to-Implant Ratio; Dental implants complications; Implant-supported single crowns; Marginal bone loss.

INTRODUCTION

Restoration of edentulous areas with implant-supported prosthetic restorations is a widely accepted alternative nowadays. One of the successful criteria for implant restorations is the stability of osseointegration and bone-to-implant contact (BIC). It is generally accepted that in physiological functional load it can be expected to have a bone loss of 1 to 1.5 mm within the first year and less than 0.2 mm every successive year (1). This process can be accelerated by mechanical, chemical and biological factors. Due to the onset of bone atrophy after teeth extraction and the limited height of available bone, it is often necessary the use implants with a smaller length than that of the restoration in the distal areas of jaws (2, 3). In such situations, the crown-to-implant (C/I) ratio is increased (Fig. 1). Elevated values of this parameter affect the vertical bone loss around the implant (4). There is still no uniform opinion regarding the optimal values of this ratio and its effect on marginal bone loss. The data of published studies are often contradictory. According to Hingsammer et al. the ratio between the crown and the implant should not exceed 1.7 in order to avoid increased early bone loss (5). Meijer et al. monitored the frequency of biomechanical complications associated with elevating this indicator. The data of the conducted study showed that there was no significant increase in marginal bone loss at values from 0.86 to 2.14 (6). This is confirmed by recent research carried out by Hämmerle et al., where it was determined that from a biomechanical point of view, it is desirable for a crown-to-implant ratio to be in the range of 0.9 to 2.2 in single restorations (7). Increasing this marker above certain limits may lead to mechanical complications due to overloading occlusal forces upon the marginal part of the alveolar bone, crest module and implant body. With its increase, the size of the non-axial forces rises, with which the crown acts as a lever arm. This creates a bending moment that carries stress to the marginal bone. Malchiodi et al. conducted a prospective study with a follow-up period of three years. The data point out that the ratio of crown height to dental implant length is the main parameter able to

influence the clinical survival of dental implants. A critical value of 3.1:1 has been ascertained in which the marginal bone loss was so great that the implant osseointegration was destroyed (8). Surprisingly, some studies have even reported feedback between the crown-to-implant ratio and marginal bone loss, recording low values at higher ratios (9). In some research, it is suggested that high values of the C/I ratios may provide a protective effect on the marginal bone (10). There are also publications according to which the extent of marginal bone loss is not related to this parameter (11,12,13,14).

It becomes clear that the crown-to-implant ratio should be subject to careful consideration in making the treatment plan in implant recovery. Its increase leads to a proportional rise in the mean stress on the retained screw and peri-implant bone. Increasing the ratio of 1:1 to 1.25:1 leads to intensifying the stress in the implant crest module by 30.1%, respectively; in the ratio 1.5:1 the stress is grown by 51.5% (15).

MATERIALS AND METHODS

In the present study, 65 partially edentulous patients of the lower jaw in the area of mandibular molars have been retrospectively traced out. The distribution of the study group is as follows: 35 women and 30 men aged between 20 and 75 years at the time of implantation. The treatment had been performed only with single implant-supported cemented crowns. The following indicators were considered.

- Anatomical characteristics in the implantation area, width, height and inclination of the available bone.
- Implant characteristics, diameter, length and mesio-distal and vestibulo-lingual inclination.
- Crown height space.
- Crown-to-implant ratio.
- Size of the marginal bone loss after the first and third years of the functional load of implant-supported

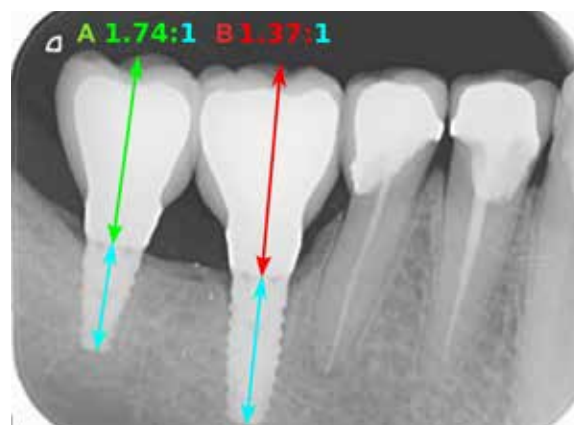


FIG. 1 Different crown-to implant ratios. A) Ratio of 1.74:1, implant length 8.00 mm. B) Ratio of 1.37: 1, implant length 10.0 mm.

prosthetic restorations.

We used the following criteria for selection and inclusion in the study.

- Cases of one missing tooth in the lower molar region;
- Patients with a width of available bone of more than 6.0 mm in the area of implantation and no periodontal diseases;
- Patients without para-functional activity;
- Non smokers.

Criteria for exclusion from the study were as follows.

- Radiotherapy.
- Untreated oral pathology or malignant tumors.
- Drug or alcohol dependence.
- Intravenous bisphosphonate therapy.
- Immunosuppression.
- Inability to maintain adequate oral hygiene.

All implantations were performed after a preliminary occlusal analysis, including a study of parafunctional activity, occlusal pattern, supraeruption, crown height space as well as inter-dental and intermaxillary relations. Preoperative scanning of the edentulous area in a central occlusion was performed by means of cone-

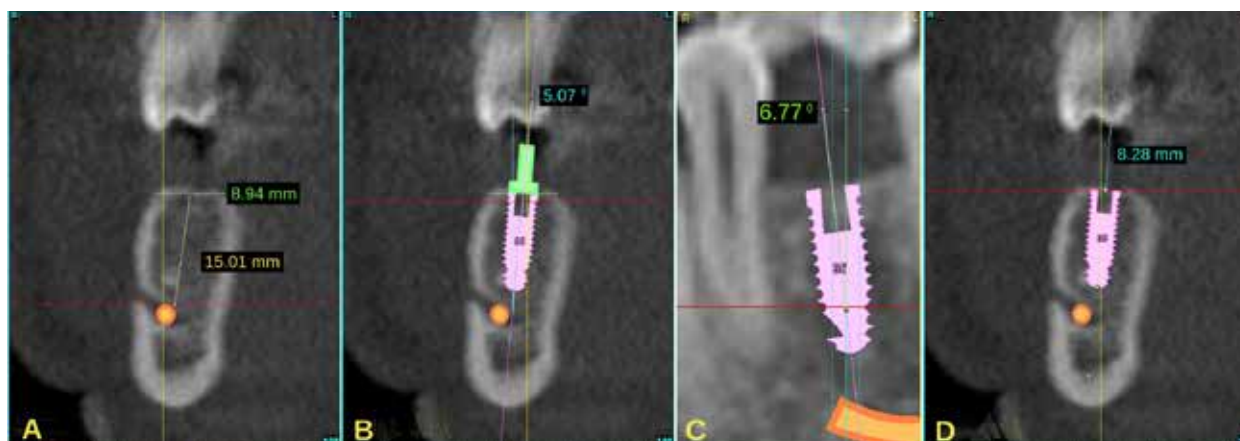


FIG. 2 Reconstructed paraxial CBCT images. Measuring of parameters of available bone: width and height (A), vestibulo-lingual (B) and mesio-distal (C) inclinations and crown height space (D).

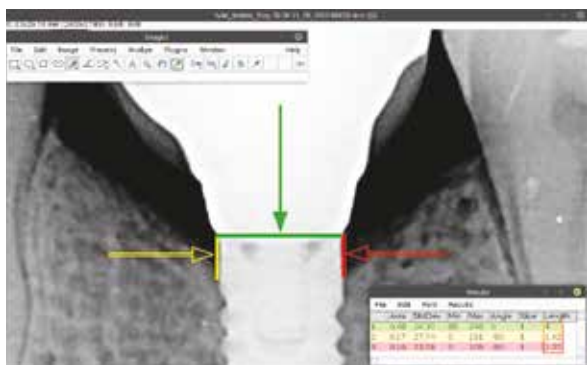


FIG. 3 Measuring the marginal bone loss from the medial (yellow arrow) and distal side (red arrow). The diameter of the implant platform is marked with a green arrow.

beam computed tomography (CBCT) (Planmeca Pro X (Planmeca Oy, Helsinki, Finland). The selection of optimal implant sites and measurements of available bone volume were made with Simplant Pro (Dentsply Sirona, Mannheim Germany). The width of the available bone was measured between the buccal and lingual bone plates along the crest of the alveolar ridge, and the available bone height was recorded from the crest of the alveolar ridge to the mandibular canal (Fig. 2A). The inclination of the planned dental implant position was measured depending on the occlusal plane in vestibulo-lingual (Fig. 2B) and in mesio-distal direction (Fig. 2C). The crown height space was measured from the crestal bone level to the crowns of the antagonist teeth (Fig. 2D). All placed implants were "bone level" type (TBR Connect and TBR Periosave M; TBR Implants group, Toulouse, France) with a diameter of 4.0 mm (Connect) and 3.9 mm (Periosave M) and lengths in the range of 8.0 to 13.0 mm.

Resorption of marginal bone was measured by means of periapical radiographs using ImageJ 1.52 (National Institutes of Health, Bethesda, Maryland, USA). Each image was calibrated individually according to the diameter of the implant platform. The distance from the implant shoulder to the level of solid contact with bone, respectively from the medial and distal sides was recorded, by registering the mean value (Fig. 3).

The statistical methods we have used are consistent with the nature of data and the nature of followed phenomena. Most of the indicators have no normal distribution, which necessitated using nonparametric methods of analysis. Descriptive methods of categorical and quantitative variables processing (mean, median, mode, standard deviation, minimum and maximum), cross tabulations, correlation analysis, as well as hypothesis testing methods were applied.

Aim of the study

The aim of current study was to determine whether the crown-to-implant ratio influences the size of the marginal bone loss around implant-supported single crowns after being functionally loaded.

RESULTS

Most of the indicators used do not have normal distribution, which necessitates the use of nonparametric analysis methods. In the present study, the width of the alveolar bone was greater than or equal to 6.0 mm, i.e. the condition for a minimum distance of 1.0 mm from the implant periphery by this indicator was strictly observed. In order to determine whether there is a difference in the level of the marginal bone loss compared to the width of the available bone Kruskal-Wallis test was used. The data from the conducted test indicate that there are no statistically significant differences between the mean ranks of the study groups: $-\chi^2(4) = 7.540, p = 0.110$.

Vestibulo-lingual inclinations are reduced to the minimum possible, taking into account the anatomical conditions in the implant area. The distribution of the cases is as follows: 0° , 40.0%, from 10 to 15° , 30.8%, from 15 to 25° , 26.2% and over 25° , 3.1%. Mesio-distal inclinations are consistent with achieving optimal positioning of the implant platform and with root inclinations of natural teeth. In most cases the inclination size is minimal: 0° – 41.5%, from zero to five degrees – 43.1%, from five to ten degrees – 13.8% and between ten and 15 degrees – 1.5%. To trace the influence of the implants inclination on the detected crestal resorption after the third year Kruskal-Wallis test was used. The results of the test showed that there was no statistically significant difference between the study groups $-\chi^2(4) = 4.749, p < 0.314$.

The data for the distribution of the crown-to-implant ratio were combined into five groups: 1.5:1, 10.8%; 1.25:1, 15.4%; 1:1, 18.5%; 1:1.25, 35.4%; 1:1.5, 20.0%. Ratios larger than 1:1 were recorded in only 17 cases (26.2%). The mean value of the followed indicator was 0.871 compared to a standard deviation of 0.279.

After the first year of the functional load, we found low levels of marginal bone loss: 32 cases with 0 mm, 32 cases with crestal resorption to 1.0 mm and 1 with 1.2 mm. Mean values of the tracing indicator was 0.254 with a standard deviation of 0.299. Recording this indicator after the third year, a slight increase in crestal resorption was found: 14 cases with 0 mm, 30 with 1.0 mm, 14 from 1.5 to 2.0 mm and one with 2.2 mm. The percentage distribution of these cases is presented in Figure 4.

Kruskal-Wallis test was applied in order to verify the hypothesis that the mean levels of marginal bone loss after the first year of functional load of the single crowns is the same in the different ratios between the length of the crown and the implant. The results showed that there were statistically significant differences between the four study groups $-\chi^2(4) = 19.92, p = 0.006$. The same test was applied to the cases with crestal resorption after the third year in relation to the different crown-to-implant ratios. In these cases, we also found statistically significant differences in the

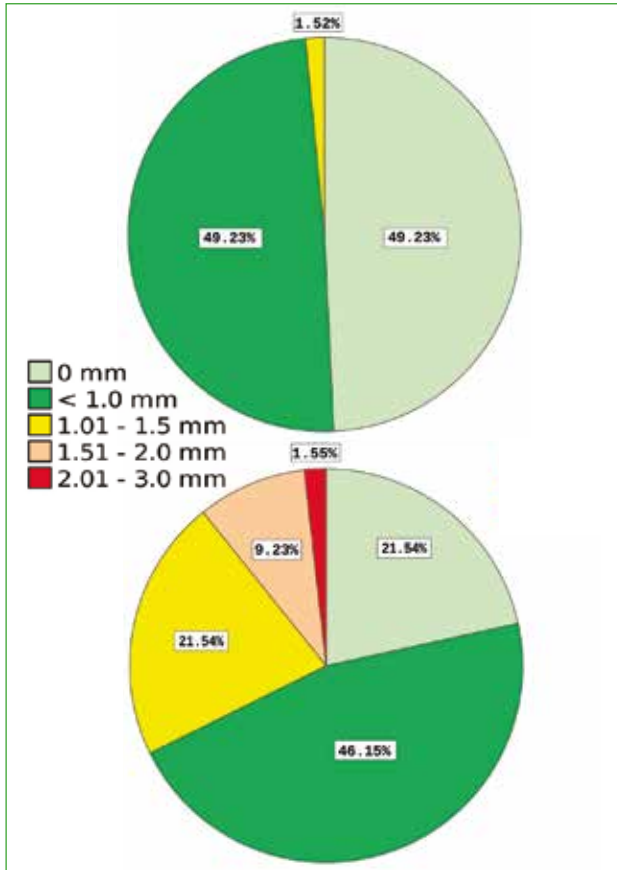


FIG. 4 Percentage distribution of marginal bone loss after first (in the left) and third (in the right) years of the functional load. A very low incidence of cases with resorption over 1.0 mm is observed after the first year. After the third year, incidence of cases with resorption to 1.0 mm is still prevalent (67.69%). Those with more than 1.00 and 1.5 mm are increasing.

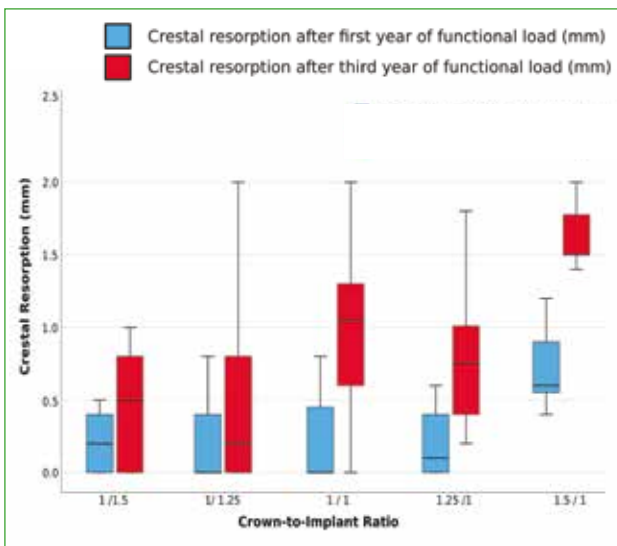


FIG. 5 Boxplot. Mean distribution of marginal bone loss after the first and after the third year among the different groups. Though all values are within the optimal range, there is a tendency for them to rise at higher crown-to-implant ratios.

mean ranks between the different groups - $\gamma^{(2)}(5) = 24.639, p < 0.001$. The distribution of the marginal bone loss compared to the crown-to-implant ratio after the first and third years of the functional load is shown in Figure 5. There is a slight increase in indicators monitored during the third year. This is most pronounced in cases when the crown-to-implant ratio is 1:1 and higher.

In order to investigate the association between the size of crestal resorption after the first and third years compared to the crown-to-implant ratio, Spearman rho rank correlation coefficient was used. The data from the conducted tests point out that there is a statistically significant relationship between the studied parameters - $\rho(65) = 0.276, p = 0.026$ - for the reported values of marginal bone loss after the first year and $\rho(65) = 0.536, p < 0.001$ for those after the third year. The correlation signs are positive, which means that the higher the crown-to-implant ratio becomes, the higher the reported values of the marginal bone loss are.

DISCUSSION

The current study results show that increasing the values of the crown-to-implant ratio has a statistically significant positive correlation with marginal bone loss around the implant. They confirm the conclusions of the study by Sotto-Maior et al. (16), in which the effect of such indicator on the distribution of occlusal stress in the implant supported prosthetic restorations is being monitored. The data in it show that 22.47% of cortical bone stress is due to increased crown-to-implant ratio. Its values rise with the increase of this indicator (16). This dependence is also described in other prospective clinical studies (2, 17). In studies with the three-dimensional finite element analysis it is also indicated that short implants create higher stress in bone around the implant (18, 19). They show that high crown-to-implant ratios affect both cortical and cancellous bone during axial and non-axial loads. Therefore, in such situations, cantilevers should be avoided (20).

Our clinical data also confirm the results of Cinar and Imirzalioglu, who determined applying the finite element method that the concentration and distribution of occlusal stress increases with the crown height (21). In a two-fold increase in the crown-to-implant ratio, the stress in von Mises' research increased by 47%, while with ratios close to 2:1, the highest stress was observed in the implant crest module (21).

The results of the present study are consistent with the data from the systematic review of the literature by Garaicoa-Pazmiño et al., where it is revealed that the crown-to-implant ratio has an effect on marginal bone loss (10). Similar results are depicted in Malchiodi et al. research in the analysis of 259 short dental implants among 136 patients for a 36-month period of time. The authors ascertained a significant correlation between the

clinical crown-to-implant ratio and the peri-implant bone loss, with the highest reported values at 2:1 ratios (8). According to other studies, these ratios show a direct relationship to peri-implant bone stress, but the absolute height of the restorative space and the implant diameter have a greater influence upon crestal resorption. Lower stress values have been recorded for large-diameter implants, even in cases with a long crown height space (22). It is essential to note that the increased height of the restorative space is directly related to the crown-to-implant ratios due to the anatomical implant length limitations in the distal parts of the jaws. On the other hand, to determine the effect of this parameter on marginal bone loss, it is necessary to isolate the influence of additional factors such as surgical technique, height of the restorative space, type, length and diameter of the implant, its localization and bone quality (23). These factors also have an effect on marginal bone loss in the implant-supported restorations (24).

CONCLUSION

Within the current study, higher-ratio C/I implants show greater marginal bone loss in comparison with lower-ratio C/I implants in the posterior areas of the mandible. From a biomechanical point of view, the crown-to-implant ratio is an important parameter that can influence the success of the implant-supported restorations and the marginal bone loss. Therefore, it is of great importance to aim at a low C/I ratio in order to avoid excessive stress in the implant-bone interface, which may lead to increased crestal bone loss or implant failure. Due to the limited amount of data, further research into the influence of crown-to-implant ratio on the marginal bone loss should be carried out under identical conditions.

Acknowledgments

We would like to thank Assoc. Prof. Milena Stoycheva, Medical University, Sofia, Faculty of Public Health, for statistical data processing.

The authors declare no financial and non-financial competing interests.

The authors declare that they received no funding.

The authors contributed equally.

REFERENCES

- Zarb G, Albrektsson T. Consensus report: Towards optimized treatment outcomes for dental implants. *J of Prosth Dent* 1998;80:641.
- Villarinho EA, Triches DF, Alonso FR, Mezzomo LAM, Teixeira ER, Shinkai RSA. Risk factors for single crowns supported by short (6-mm) implants in the posterior region: A prospective clinical and radiographic study. *Clin Implant Dent Relat Res* 2017;19:671-680.
- Ozgur GO, Kazancioglu HO, Demirtas N, Deger S, Ak G. Risk Factors Associated With Implant Marginal Bone Loss: A Retrospective 6-Year Follow-Up Study. *Implant Dent* 2016;25:122-7.
- Dalago HR, Schuldt Filho G, Rodrigues MA, Renvert S, Bianchini MA. Risk indicators for Peri-implantitis. A cross-sectional study with 916 implants. *Clin Oral Implants Res* 2017;28:144-150.
- Hingsammer L, Watzek G, Pommer B. The influence of crown-to-implant ratio on marginal bone levels around splinted short dental implants: A radiological and clinical short term analysis. *Clin Implant Dent Relat Res* 2017;19:1090-1098.
- Meijer HJA, Boven C, Delli K, Raghoobar GM. Is there an effect of crown-to-implant ratio on implant treatment outcomes? A systematic review. *Clin Oral Implants Res* 2018;29 Suppl 18:243-252.
- Hämmerle CHF, Cordaro L, Alccayhuaman KAA, Botticelli D, Esposito M, Colomina LE, Gil A, Gulje FL, Ioannidis A, Meijer H, Papageorgiou S, Raghoobar G, Romeo E, Renouard F, Storelli S, Torsello F, Wachtel H. Biomechanical aspects: Summary and consensus statements of group 4. The 5th EAO Consensus Conference 2018. *Clin Oral Implants Res* 2018;29 Suppl 18:326-331.
- Malchiodi L, Cucchi A, Ghensi P, Consonni D, Nocini PF. Influence of crown-implant ratio on implant success rates and crestal bone levels: a 36-month follow-up prospective study. *Clin Oral Implants Res* 2014;25:240-251.
- Lee KJ, Kim YG, Park JW, Lee JM, Suh JY. Influence of crown-to-implant ratio on perimplant marginal bone loss in the posterior region: A five-year retrospective study. *J Periodontol* 2012;42:231-236.
- Garaicoa-Pazmiño C, Del Amo FS-L, Monje A et al. Influence of crown/implant ratio on marginal bone loss: A systematic review. *J Periodontol* 2014;85:1214-1221.
- Nunes M, Almeida RF, Felino AC, Malo P, de Araújo Nobre M. The Influence of Crown-to-Implant Ratio on Short Implant Marginal Bone Loss. *Int J Oral Maxillofac Implants* 2016;31:1156-63.
- Guljé FL, Raghoobar GM, Erkens WA, Meijer HJ. Impact of crown-implant ratio of single restorations supported by 6-mm implants: A short-term case series study. *Int J Oral Maxillofac Implants* 2016;31:672-5.
- Ravidà A, Barootchi S, Alkanderi A, Tavelli L, Suárez-López Del Amo F. The Effect of crown-to-implant ratio on the clinical outcomes of dental implants: a systematic review. *Int J Oral Maxillofac Implants* 2019 Feb 19.
- Ghariani L, Segaan L, Rayyan MM, Galli S, Jimbo R, Ibrahim A. Does crown/implant ratio influence the survival and marginal bone level of short single implants in the mandibular molar? A preliminary investigation consisting of 12 patients. *J Oral Rehabil* 2016;43:127-35.
- Verri FR, Batista VE, Santiago JF Jr, Almeida DA, Pellizzer EP. Effect of crown-to-implant ratio on peri-implant stress: a finite element analysis. *Mater Sci Eng C Mater Biol Appl* 2014;45:234-40.
- Sotto-Maior BS, Senna PM, da Silva WJ, Rocha EP, Del Bel Cury AA. Influence of crown-to-implant ratio, retention system, restorative material, and occlusal loading on stress concentrations in single short implants. *Int J Oral Maxillofac Implants* 2012;27:e13-8.
- Ramos Verri F, Santiago Junior JF, de Faria Almeida DA, de Oliveira GB, de Souza Batista VE, Marques Honório H, Noritomi PY, Pellizzer EP. Biomechanical influence of crown-to-implant ratio on stress distribution over internal hexagon short implant: 3-D finite element analysis with statistical test. *J Biomech* 2015;48:138-45. Epub 2014 Oct 30.
- Güngör H. Influence of Crown-to-Implant Ratio on Stress Concentration of Fixed Dental Prosthesis in Shortened Dental Arch Concept. *Dent Implants Dentures* 2016;1:112.
- De Moraes SL, Verri FR, Santiago JF Jr, Almeida DA, de Mello CC, Pellizzer EP. A 3-D finite element study of the influence of crown-implant ratio on stress distribution. *Braz Dent J* 2013;24:635-41.
- Maminskas J, Puisys A, Kuoppala R, Raustia A, Juodzbaly G. The Prosthetic Influence and Biomechanics on Peri-Implant Strain: a Systematic Literature Review of Finite Element Studies. *J Oral Maxillofac Res* 2016;7:e4.
- Cinar D, Imirzalioglu P. The effect of three different crown heights and two different bone types on implants placed in the posterior maxilla: Three-dimensional finite element analysis. *Int J Oral Maxillofac Implants* 2016;31:e1-10.
- Bayraktar M, Gultekin BA, Yalcin S, Mijiritsky E. Effect of crown to implant ratio and implant dimensions on periimplant stress of splinted implant-supported crowns: a finite element analysis. *Implant Dent* 2013;22:406-413.
- Kim YK, Yun PY, Yi YJ, Bae JH, Kim SB, Ahn GJ. One-Year Prospective Study of 7-mm-Long Implants in the Mandible: Installation Technique and Crown/Implant Ratio of 1.5 or Less. *J Oral Implantol* 2015;41:e30-5.
- Anitua E, Alkhraisat MH. 15-year follow-up of short dental implants placed in the partially edentulous patient: Mandible Vs maxilla. *Ann Anat* 2019;222:88-93.